



**HP WHITE
LABORATORY**

An Intertek Company

DEA Ballistic Shield Testing
Protocol v2.0



SOLICITATION NUMBER
D-14-TR-0093

CONTRACTING AGENCY
Drug Enforcement
Administration (DEA)

OFFER DUE DATE/TIME
10-JUL-2014

SAMPLE RECEIPT DEADLINE
4-JUL-2014

TIME TO COMPLETE TESTS
2 days

PRICE
Call +1.410.838.6550



INDEPENDENT TESTING

Version 1
29-MAY-2014

Summary of Test Requirements

DEA Designation	Cartridge Specs	Velocity (+/- 75 fps)	Shots	Quadrant
TR01	7.62 x 51mm M80 Ball, 149 gr	2750	5	Q1
TR02	7.62 x 39mm MSC, 123 gr	2400	5	Q2
TR03	5.56 X 45mm Federal, 62 gr Tactical Bonded	2800	5	Q3
TR04	5.56 x 45mm M855 (Green Tip), 62 gr	3050	5	Q4

DEA Shot Quadrants

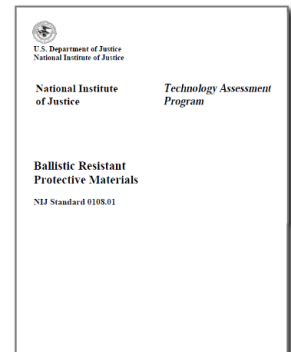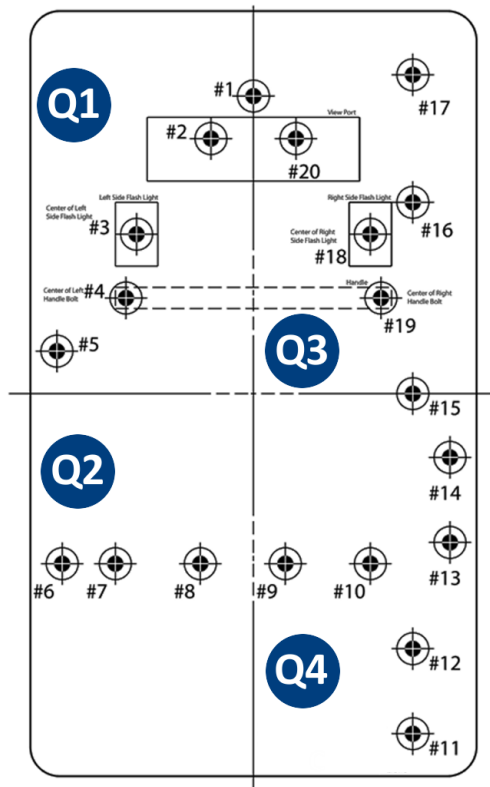

Compliance with
NIJ 0108.01
is also required.
Schedule testing
today at HP White.

Ship Samples to: **HP White Laboratory, Inc.**
3114 Scarborough Road
Street, MD 21154
+1.410.838.6550

Contact us to learn more
info@hpwhite.com

